

Title	小さなプローブ分子を用いた単層カーボンナノチューブ電界効果トランジスタバイオセンサ
Author(s)	Nguyen, Tung Thanh
Citation	
Issue Date	2019-03
Type	Thesis or Dissertation
Text version	ETD
URL	<a href="http://hdl.handle.net/10119/15796">http://hdl.handle.net/10119/15796</a>
Rights	
Description	Supervisor:高村 禪, 先端科学技術研究科, 博士

氏名	NGUYEN, Tung Thanh		
学位の種類	博士(マテリアルサイエンス)		
学位記番号	博材第 462 号		
学位授与年月日	平成 31 年 3 月 22 日		
論文題目	Single-walled carbon nanotube field-effect transistor biosensor using small probe molecules		
論文審査委員	主査	高村 禅	北陸先端科学技術大学院大学 教授
		水田 博	同 教授
		平塚 祐一	同 准教授
		筒井 秀和	同 准教授
		前橋 兼三	東京農工大学 教授


## 論文の内容の要旨

### Background:

Field-effect transistor (FET)-based biosensors offer many advantages such as real-time, label-free, fast response, portability, and high density integration in addition to its high sensitivity. Among FET-based biosensors, single-walled carbon nanotube field-effect transistor (SWCNT-FET)-based biosensor manifests a promising candidate thanks to its quasi-one dimensional SWCNT channel. Every atom is located onto the surface of SWCNT; therefore it is extremely sensitive to small change of surrounding environment. However, FET-based biosensors in general and SWCNT-FET-based biosensor in particular face a critical issue of the Debye shield (physical length of approximately 1 nm induced by counterions in physiological environment) which limits the selection of probe molecules. Besides, conventional probe molecule such as antibody – a product of *in vivo* biological protocol, which is large in size (10 – 12 nm) and suffered from batch to batch activity variation, critical storage condition and high cost, is not suitable for FET-based biosensors. To overcome this problem, the small probe molecule is utilized to bring the binding event to the vicinity of sensing surface of FET in order to enhance the field effect from charged biomolecule target, hence improving the sensitivity of the sensor. In the previous study, small fragment of antibody (such as Fab'2 fragment, Fab fragment) and DNA aptamer were used as small probe molecules integrated into SWCNT-FET biosensor. As a result, the sensitivity of SWCNT-FET sensor could be improved remarkably. In this study, we demonstrated the utilization of small probe molecules such as peptide aptamer and glutamate-binding protein (GBP) integrated with SWCNT-FET. The peptide aptamer is *in vitro* chemically synthesized. Therefore,

its activities are uniform regardless of batch with extended storage time; synthesis is quicker and inexpensive; especially it can be flexibly modified to approach wide variety of target while antibody is limited. Compared with DNA aptamer which is made by a combination of 4 nucleic acids, peptide aptamer is a mimic form of a variable loop of antibody, hence peptide aptamer possesses higher specific affinity. The GBP exhibits rapid recognition to transient Glutamate (Glu) – a key neurotransmitter in a central nervous system. Since the current methods for Glu detection are suffered from temporal and spatial resolutions, therefore GBP is a promising candidate to integrate with SWCNT-FET for studying fast process of Glu transmission.

**Aim:** In this study, we demonstrated the utilization of small probe molecules such as peptide aptamer and GBP integrated with SWCNT-FET (Figure 1). The peptide aptamer was integrated with SWCNT-FET to develop highly selective and sensitive biosensor. The GBP was combined with network SWCNT-FET to develop a sensor for real-time monitoring of transient Glu, aiming for neuroscience application.

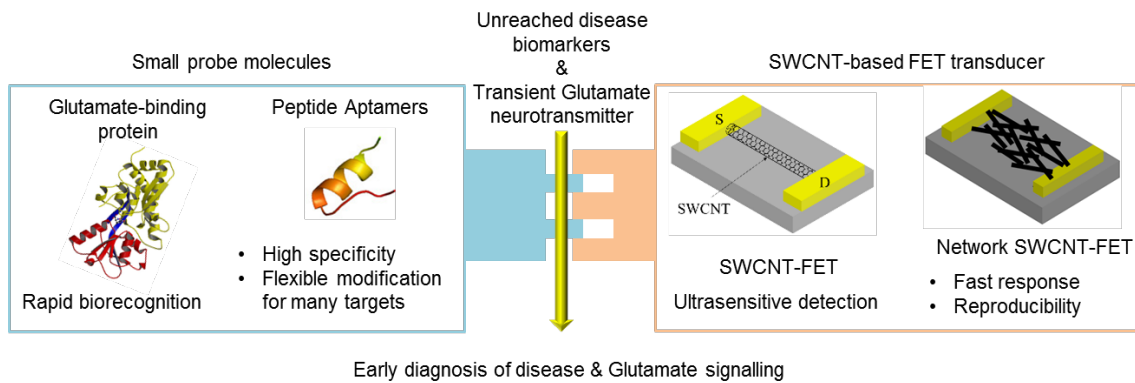


*Figure 1: The integration of small probe molecules with SWCNT-based FET.*

## **Experimental:**

### **1. Peptide aptamer-modified CVD-type SWCNT-FET biosensor**

First, SWCNT-FETs were fabricated on the Si/SO<sub>2</sub> substrate by growing SWCNTs on Co catalyst using catalytic alcohol chemical vapour deposition (CVD). We call this CVD-type SWCNT-FET. The novel peptide aptamer that specifically recognizes Cathepsin E (CatE) – a useful prognostic biomarker for cancer diagnosis, was utilized as probe molecule. The peptide aptamer was immobilized onto the SWCNT channel via 1-pyrenebutanoic acid succinimidyl ester (PBASE) linker, following by blocking the unreacted PBASE linker with ethanolamine (Figure 2). The fabricated peptide aptamer-modified CVD-type SWCNT-FET sensors were subjected to each CatE concentrations in 1X PBS pH 10 and 10-times diluted human serum, respectively, followed by rinsing thoroughly with 0.0005X PBS pH 4, and then dried with nitrogen

gas. Finally, a Parafilm cavity was attached to the device to contain the 0.0005X PBS pH 4 during electrical measurements. To check the selectivity, the fabricated sensors were exposed to the interference molecules such as bovine serum albumin (BSA) and Cathepsin K (CatK).

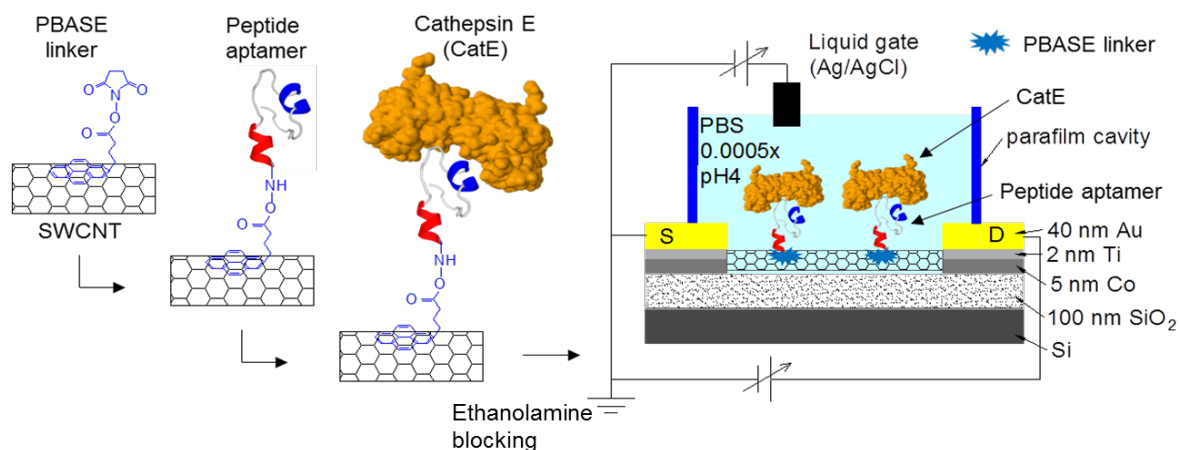

*Figure 2: The immobilization of peptide aptamer onto the surface of SWCNT and the operating setup of liquid-gated CVD-type SWCNT-FET device for CatE detection.*

## 2. GBP-modified network SWCNT-FET biosensor

To simplify the process of device fabrication and improve the reproducibility, a semiconducting SWCNT solution was used for the deposition of random network SWCNT channel. This technique is simple and fast, allowing a direct control of network density of SWCNT channel and hence the transistor characteristics. We call this network SWCNT-FET. Then the network SWCNT was functionalized by immobilization of the GBP probe molecule using PBASE linker. Then a Parafilm cavity was attached to the device to contain 0.01X PBS pH 7.5. The fabricated GBP-modified network SWCNT-FET sensor was subjected to various Glu concentrations for real-time measurement. To check the selectivity, the fabricated sensor was exposed to interference molecule such as Dopamine – another neurotransmitter.

### Results and discussion:

#### 1. Peptide aptamer-modified CVD-type SWCNT-FET biosensor

Figure 3 (a) shows the response of fabricated peptide aptamer-modified CVD-type SWCNT-FET sensor to CatE in 1X PBS buffer pH 10. The conductance of SWCNT channel decreased with increasing CatE concentrations from 0.1 to 0.6 ng/mL. This decrease in conductance is due to the positive charge of CatE at pH 4 which induces the decrease of hole carrier density inside SWCNT channel by field effect. There was no change in conductance for the CatE concentration above 0.6 ng/mL because all peptide aptamer probe molecules were occupied. There was no significant response of the

CVD-type SWCNT-FET device, which was modified with PBASE linker, followed by blocking with ethanolamine, to 1 ng/mL CatE (Figure 3 (b)). This result indicated that the nonspecific binding between CatE and SWCNT was suppressed. Figure 3 (c) shows the comparison between the responses of the fabricated sensors to CatE, CatK and BSA. The result indicates that the fabricated sensors strongly respond to CatE, but negligibly respond to CatK and BSA, exhibiting the specificity of fabricated sensor.

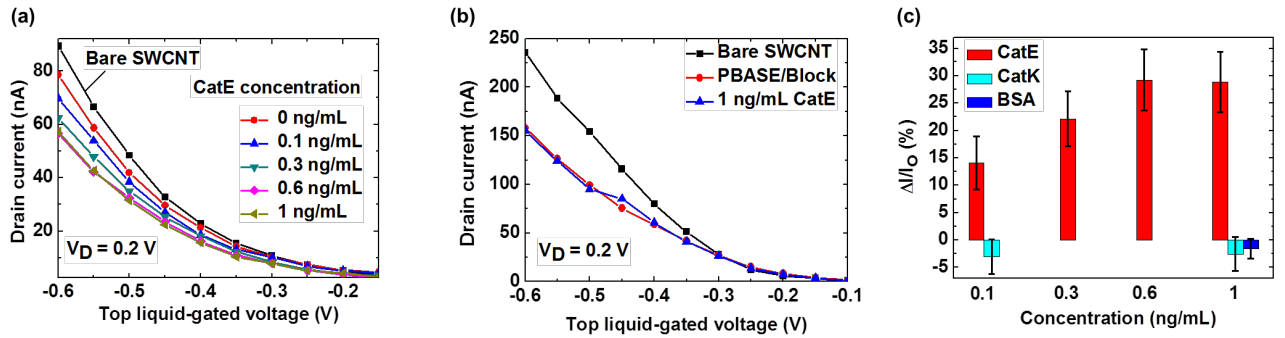


Figure 3: The electrical characteristics of CVD-type SWCNT-FET modified with (a) and without peptide aptamer probe molecule (b) responding to CatE; and (c) the response of peptide aptamer-modified CVD-type SWCNT-FET to CatE, CatK and BSA.

Using the fabricated sensor, we proceed to detect CatE in 10-times diluted human serum. As a result, the sensor responds to CatE from 10 to 100 ng/mL (Figure 4 (a)). In the calibration curve in Figure 4 (b), the intensity of response signals increased with increasing CatE concentration from 10 to 60 ng/mL because of the positive charge of CatE. The lowest detectable CatE of 10 ng/mL in human serum is three times of magnitude lower than that of a conventional ELISA system using a similar peptide aptamer [1]. These results indicated that the use of small peptide aptamer is an effective strategy for realizing highly sensitive and selective FET-based biosensors. Our demonstrated sensor could be a promising platform for near-patient testing and point-of-care testing applications.

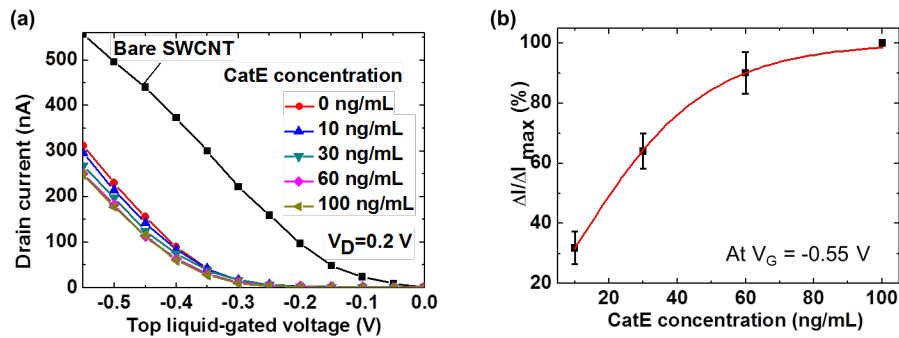


Figure 4: Quantitative detection of CatE in 10-times diluted human serum.

## 2. GBP-modified network SWCNT-FET biosensor

Figure 5 (a) shows the response of network SWCNT-FET with GBP probe molecule to Glu from 10 to 50  $\mu\text{M}$  (black line) whereas the network SWCNT-FET without GBP shows no significant response to this range of Glu concentrations (red line). This result indicated the nonspecific binding between Glu and network SWCNT was suppressed and the increase in drain current was originated from the binding between GBP and Glu. The increase in drain current is due to the negative charge of Glu and the conformational change of GBP which induces the increase in hole carrier density inside network SWCNT channel. The sharp decrease in drain current at 100  $\mu\text{M}$  is due to the decreased pH by excessive Glu. The fabricated GBP-modified network SWCNT-FET exhibited no significant response to Dopamine (Figure 5 (b)), indicating the high selectivity property of fabricated sensor. These results indicated that our sensor could be a promising candidate for real-time monitoring of Glu at micromolar range which is sufficient for studying Glu signalling.

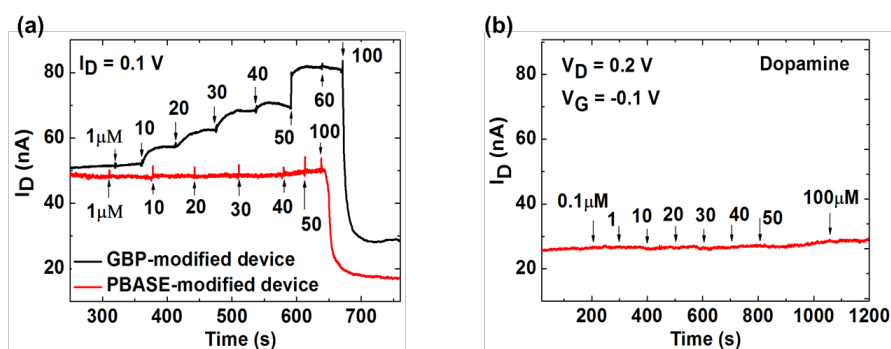


Figure 5: (a) Response of network SWCNT-FET with (black line) and without (red line) GBP to Glu; and (b) Response of GBP-modified network SWCNT-FET to Dopamine.

### Conclusion:

We have successfully demonstrated, for the first time, the integration of small probe molecules (peptide aptamer and GBP) into SWCNT-based FETs. The integration of peptide aptamer with CVD-type SWCNT-FET could achieve highly sensitive and specific detection of CatE. The integration of GBP with network SWCNT-FET could monitor Glu at micromolar range in real-time. The proposed platforms are promising for clinical application as well as neuroscience study, and be applicable for various target biomarkers.

### References:

- [1] Kitamura, K. et al. Peptide Aptamer-Based ELISA-Like System for Detection of Cathepsin E in Tissues and Plasma. *J. Mol. Biomark. Diagn.* 2, 1, <https://doi.org/10.4172/2155-9929.1000104> (2011).

**Keywords:** SWCNT-FET, peptide aptamer, Cathepsin E, Glutamate-binding protein, Glutamate.

## 論文審査の結果の要旨

本論文は、Single-walled carbon nanotube (SWCNT) をチャネル材料に用いた電界効果トランジスタ (FET) において、デバイ遮蔽と低再現性という原理的に大きな問題に向き合い、より実用的なセンサデバイスを目指すための具体的手法の確立を試みたものである。SWCNT-FET 型のバイオセンサは、その微小性、高速応答性から、生体分子のダイナミックな応答を計測できるセンサとして注目されていたが、電荷応答型のセンサのため、電解質溶液内ではデバイ遮蔽により感度が低下する。これを避けるには、より小さなプローブ分子を用いることが有効である。本研究では、ペプチドアプタマをプローブに用い、癌マーカーであるカテプシン E の高感度な検出系を構築しその有効性の実証を試みた。また CNT はカイラリティの多様性から原理的に再現性が低い。そこで予め作成された半導体型の CNT のみを塗布したネットワーク型の FET を用い、その高速応答性を活して、神経伝達物質である Glutamate の計測系の構築を目指した。

第 1 章では、SWCNT-FET を用いたバイオセンサの現状と問題点についてまとめ、本研究の課題を明確化した。

第 2 章では、バイオセンサに組み込むことができる SWCNT-FET の設計と、作成、その特性の評価を行った。ここでは、より高感度な測定が期待できる、従来型の化学気相成長(CVD)法で作成する SWCNT-FET に加え、より高再現性が期待できる市販の半導体 SWCNT を塗布して作成するネットワーク型の SWCNT-FET を作成し、期待通りの基礎特性を確認した。

第 3 章では、CVD 作成型 SWCNT-FET に、ペプチドアプタマをプローブとして初めて組み合わせ、カテプシン E の計測系を構築した。従来の抗体を用いた測定系と比べ、3~4 桁の高感度化を達成し、また同じペプチドアプタマを用いた ELISA と比べても 3 桁の高感度化を達成した。

第 4 章では、ネットワーク型の SWCNT-FET と Glutamate binding protein (GBP)を用い、Glutamate の測定系を構築した。10-50 $\mu$ M の範囲で、選択的な Glutamate のリアルタイム計測に成功した。

以上、本論文は、SWCNT-FET を用いたバイオセンサにおいて、大きな問題点であったデバイ遮蔽と低再現性の問題を扱い、ペプチドアプタマや GBP を初めて組み合わせることで、カテプシン E や Glutamate という具体的な測定系においてその有用性を実証したものであり、学術的に貢献するところが大きい。よって博士 (マテリアルサイエンス) の学位論文として十分価値あるものと認めた。